




# Valar Peptides

## Certificate of Analysis (CoA)

|                          |                                    |
|--------------------------|------------------------------------|
| <b>Product:</b>          | BPC157 & TB500                     |
| <b>Quantity:</b>         | 5 mg / 5 mg                        |
| <b>Batch/Lot No.:</b>    | BT5-03-814-n086                    |
| <b>Date of Analysis:</b> | 14 July 2025                       |
| <b>Instrument:</b>       | Agilent 1260 HPLC and Thermo (MK3) |

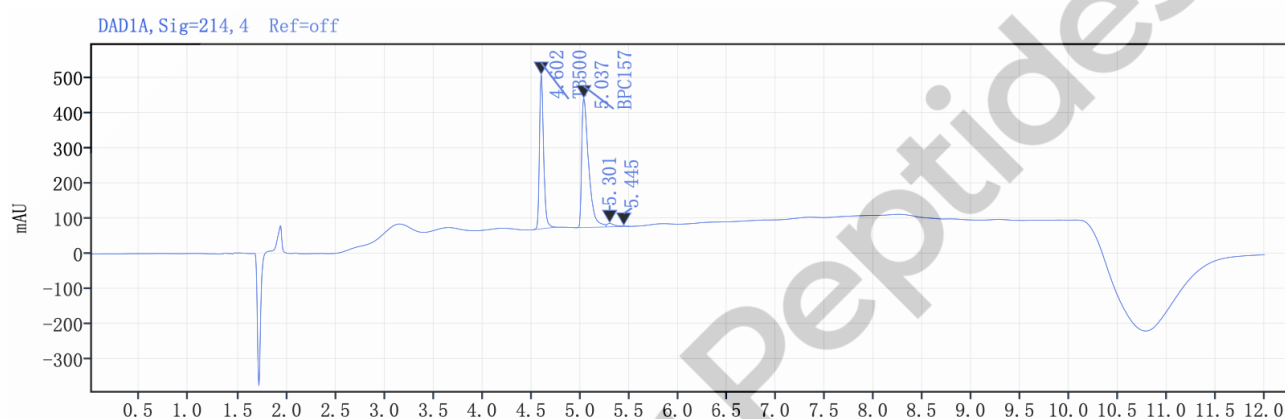

### Quality Control

| Test Parameter                  | Method            | Specification                         | Result   |
|---------------------------------|-------------------|---------------------------------------|--|
| Identification (Retention Time) | Visual inspection | White to off-white lyophilized powder | White to off-white lyophilized powder (conforms) |
| Identification (Retention Time) | HPLC              | ±0.2 min of Standard                  | Conforms   |
| Purity (by HPLC, % area)        | HPLC              | ≥ 99.0%                               | 99.03%   |
| Net Peptide Quantity            | HPLC              | 5 mg / 5 mg                           | 5.83 mg / 6.04 mg                                |
| Endotoxin                       | LAL               | ≤ 0.5 EU/mg                           | Conforms   |

Authorized by: Matt C.  
Matt C.  
Head of Quality Control