




Valar Peptides

Certificate of Analysis (CoA)

Product:	BPC157, TB500 and GHK-Cu (GLOW)
Quantity:	10 mg / 10 mg / 50mg
Batch/Lot No.:	GL05-03-814-f470
Date of Analysis:	01 August 2025
Instrument:	Agilent 1260 HPLC and Thermo (MK3)

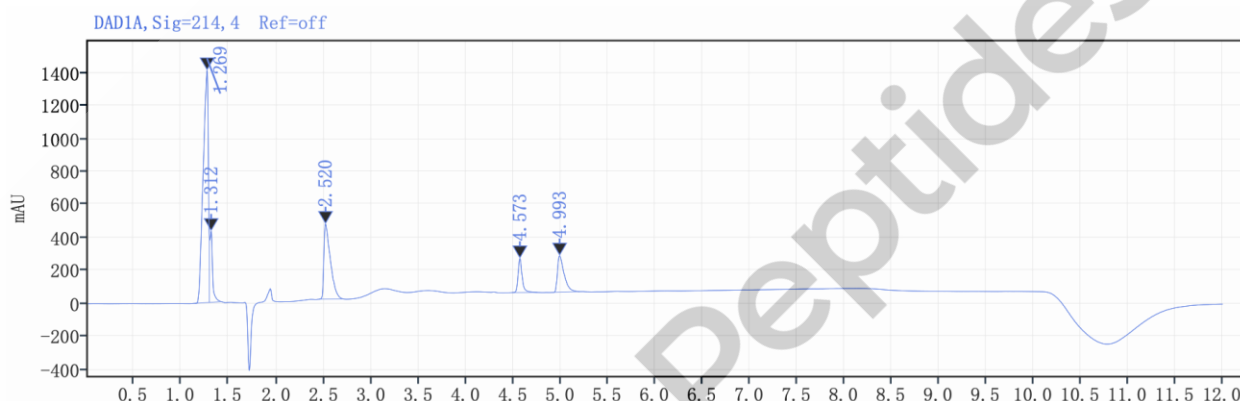

Quality Control

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	Blue to off-blue lyophilized powder	Blue to off-blue lyophilized powder (conforms)
Identification (Retention Time)	HPLC	± 0.2 min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	$\geq 99.0\%$	99.02%
Net Peptide Quantity	HPLC	10 mg / 10 mg / 50mg	10.22 mg / 11.82 mg / 65.37 mg
Endotoxin	LAL	≤ 0.5 EU/mg	Conforms

Authorized by: Matt C.
Matt C.
Head of Quality Control