




Valar Peptides

Certificate of Analysis (CoA)

Product:	Cagrilintide and Semaglutide
Quantity:	5mg / 5mg
Batch/Lot No.:	CS05-03-814-n237
Date of Analysis:	26 August 2025
Instrument:	Agilent 1260 HPLC and Thermo (MK3)

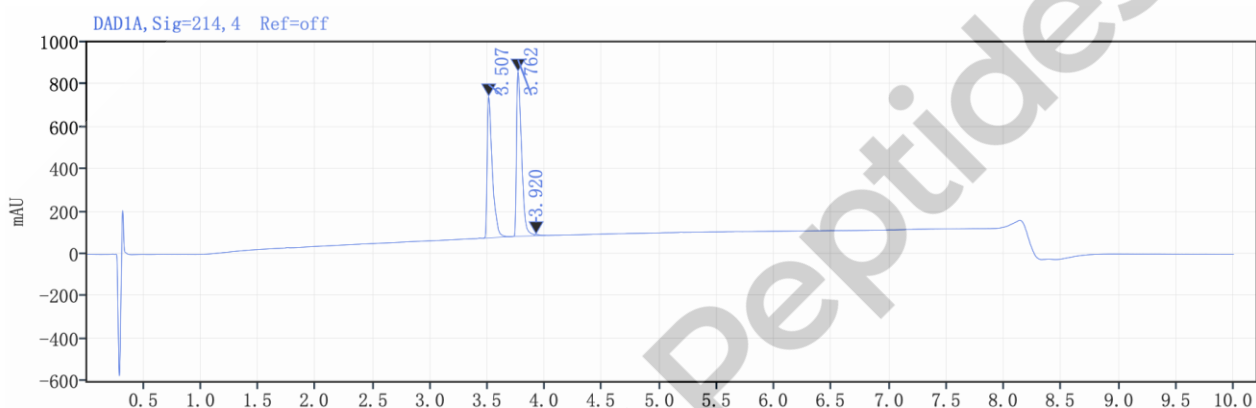

Quality Control

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	White to off-white lyophilized powder	White to off-white lyophilized powder (conforms)
Identification (Retention Time)	HPLC	± 0.2 min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	$\geq 99.0\%$	99.63%
Net Peptide Quantity	HPLC	5 mg / 5 mg	8.31 mg / 6.44 mg
Endotoxin	LAL	≤ 0.5 EU/mg	Conforms

Authorized by: 
Matt C.
Head of Quality Control